

Monoclonal antibody to C-reactive protein, clone 6F6, hlgG1

Catalogue #	R1-260-100
Immunogen:	Native human C-reactive protein
Immunogen Description:	Human native C-reactive protein
Source:	Human
Clonality:	Human monoclonal
Clone:	6F6
Class:	hlgG1
Application:	ELISA, CLIA
Kd:	3.570 x 10-11 M
Purification:	Produced recombinantly using CHO-based cell line (expressed by QMCF technology). Purified using protein A affinity chromatography followed by desalting
Purification: Purity:	line (expressed by QMCF technology). Purified using protein A affinity chromatography followed
	line (expressed by QMCF technology). Purified using protein A affinity chromatography followed by desalting
Purity:	line (expressed by QMCF technology). Purified using protein A affinity chromatography followed by desalting >90%
Purity: Concentration:	line (expressed by QMCF technology). Purified using protein A affinity chromatography followed by desalting >90% 1 mg/ml
Purity: Concentration: Buffer:	line (expressed by QMCF technology). Purified using protein A affinity chromatography followed by desalting >90% 1 mg/ml PBS, pH 7.4 LabChip protein analysis, analytical SEC, Octet


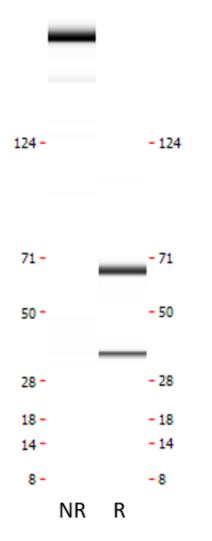


Figure 1. CE-SDS virtual gel output (LabChip GX) for monoclonal antibody to C-reactive protein, clone 6F6 under non-reduced (NR, left) and reduced (R, right) conditions.

Peak #	RT (min)	Estimated Mw (Da)*	Area	Area %
1	7.420	359333	28.11	1.03
2	8.908	131568	2699.35	98.97

Chromatogram

ICO230227 ICO0280-A01_pur_prod_final_1, DAD 220 nm

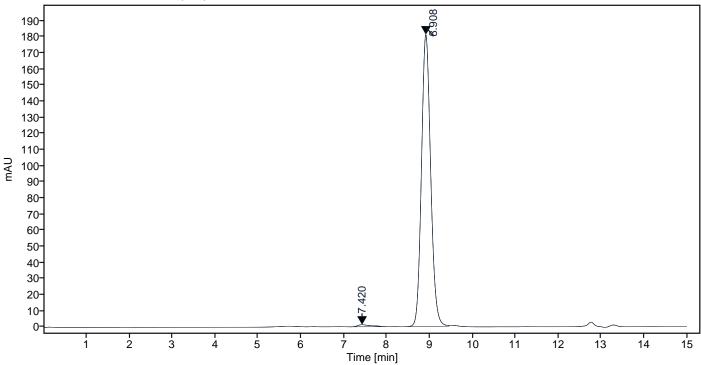


*Calculated using calibration curve obtained from AdvanceBio SEC 300A Protein Standard (p/n 5190-9417) retention times. Peaks with integrated areas below 0.5% of the calculated values were excluded from analysis.

Figure 2. Analytical SEC of final product.

Peak #	RT (min)	Estimated Mw (Da)*	Area	Area %
1	7.434	350364	21.11	1.03
2	8.907	132648	2020.68	98.97

Chromatogram

ICO230227 ICO0280-A01_pur_prod_final_1 3x, DAD 220 nm

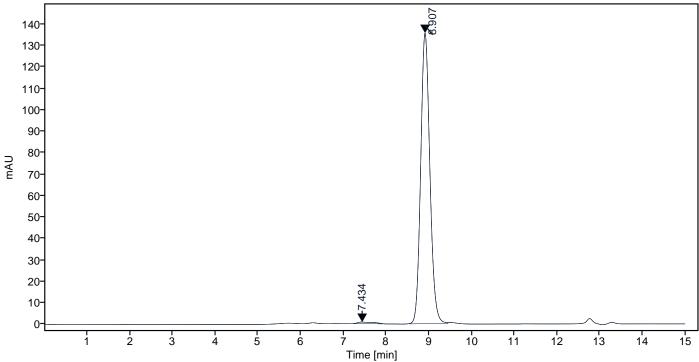

*Calculated using calibration curve obtained from AdvanceBio SEC 300A Protein Standard (p/n 5190-9417) retention times. Peaks with integrated areas below 0.5% of the calculated values were excluded from analysis.

Figure 3. HPLC analytical SEC after 3 freeze-thaw cycles.

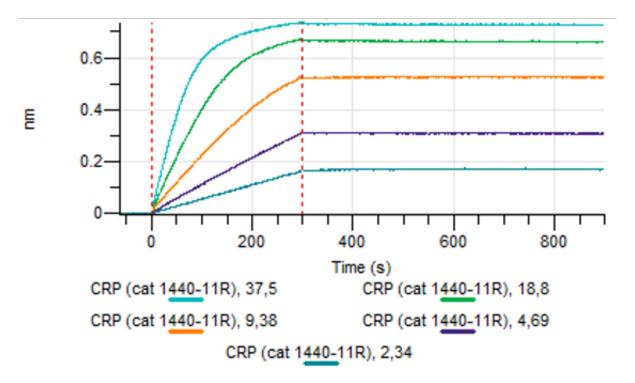


Figure 4. Octet BLI analysis, antibody was loaded on sensor for capture of C-reactive protein in different concentrations.